OCT 3 1 2001

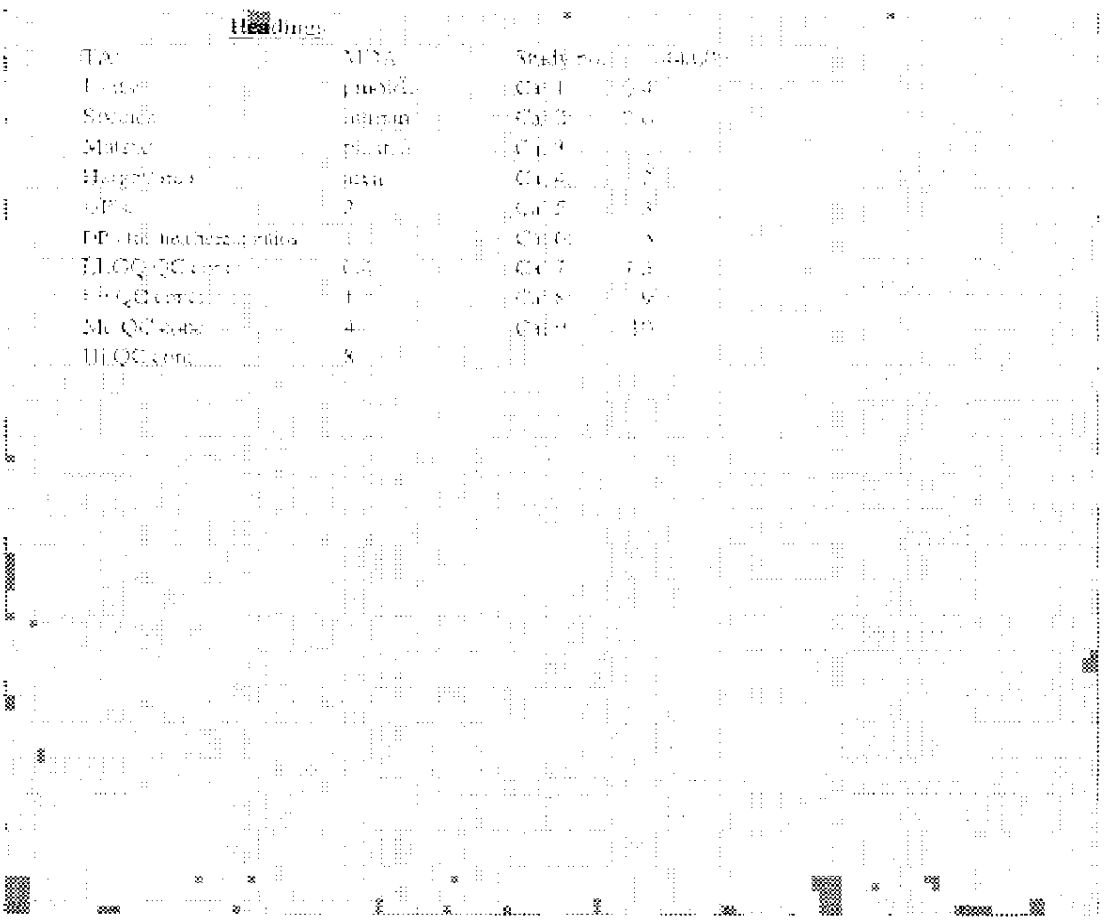

PM3006635959

Source: https://www.industrydocuments.ucsf.edu/docs/rycj0001

Footnotes from SOP 66 Rev 1: Batch annotation

- [illegible] = Above data system
- AR = Anomalous result
- BDS = Below data system
- CO = Confirms original result
- DNU = Data not used
- DNR = Data not required
- HI = High internal standard
- IM = Instrument malfunction (add reason if known)
- IP = Interferent peak
- IS = Insufficient sample
- LI = Low internal standard
- M = This result is a median value
- ME = Mis-extraction
- MI = Mis-injection
- NR = No result
- NS = No sample taken/received
- OR = Over range
- PC = Poor chromatography
- PF = Poor fit with rest of regression (excluding standard improves the correlation coefficient / curve [illegible]
- PF = Poor fit, calibration standard outside acceptance criteria
- PP = Positive predose
- PS = Poor sensitivity
- SA = Sample dropped/spilt/spoilt during preparation (Lab accident)
- SE = Spiking error
- UR = Under range (when LLOQ raised)
- Values in parentheses calculated omitting anomalous/outlying result

Source: https://www.industrydocuments.ucsf.edu/docs/rycj0001